

High-Resolution Analysis of Intact Triglycerides by Reversed Phase HPLC Using the Agilent 1290 Infinity LC UHPLC System

Application Note

Food, Hydrocarbon Processing

Authors

Michael Woodman
Agilent Technologies, Inc.
2850 Centerville Road
Wilmington, DE 19808
USA

Abstract

The Agilent 1290 Infinity LC System with ultraviolet/visible (UV/VIS) Diode Array detection (DAD) is used to analyze triglycerides in soybean oil under non-aqueous reversed phase gradient conditions. The Agilent 1290 Infinity LC System was used for the chromatographic separation of the sample on 3.0 and 2.1 mm id C18 columns, of various lengths, with 1.8- μm packing materials prepared in 600 bar (9000 psi) or special 1200 bar (18,000 psi) configurations. The ability of the Agilent 1290 Infinity LC System to operate with long, high resolution columns is demonstrated with isopropanol (IPA) or methyl tert butyl ether (MTBE) as the strong solvent and acetonitrile as the weak component of the mobile phase mixture.



Agilent Technologies

Introduction

The analysis of intact triglycerides from animal or vegetable sources has many practical uses including understanding the chemical composition of the triglyceride, assessing fuel potential, and understanding lipid metabolism and behavior in living systems. The general conditions for successful analysis of these components by high-performance liquid chromatography (HPLC) include gradient elution and low-wavelength monitoring of the overall separation. Because triglycerides have relatively few chromophores it is also beneficial to use evaporative light scattering detectors (ELSD) or mass spectrometers to facilitate other views of the separation.

During the development of this application, we analyzed a number of vegetable oils from various sources including soy, corn, rice bran, safflower, grape seed, olive, and palm oil. Because of the wide abundance of soybean oil in the United States and its growing significance in the production of bio-fuels, most of this work was standardized on maximizing the resolution of soybean oil triglycerides. These general conditions, however, are also suitable for a wide variety of samples including samples from animal lipid sources.

Intact triglycerides generally have very low water solubility and as such are commonly separated by normal phase chromatography, which separates species largely based on differences in polar functional groups, or by reversed phase chromatography operating in a non-aqueous mode of separation, which has more selectivity for small differences on carbon character such as chain length or unsaturation.

According to information published by Perkins [1] the predominant fatty acids, which are the building blocks of triglycerides on a glycerol backbone, found in soybean oil are myristic (14:0), palmitic (16:0), oleic (18:1), linoleic (18:2) and linolenic (18:3). Many other minor fatty acids are also present and because all of the fatty acids are randomly constructed into triglycerides, an extensive permutation of fatty acid sub-structure is obviously possible. Because the predominant difference between fatty acids consists of carbon chain length and number of double bonds, most of the diversity in triglycerides is found in the rather non-polar organic structural features. As a result, reversed phase chromatography is most useful for this application. Triglycerides have extremely poor solubility in water so one normally chooses either a high organic starting position, with respect to the aqueous content or, as in this work, a completely non-aqueous separation environment.

The typical structure of a triglyceride is shown in Figure 1. [2]

In this example, from top to bottom, palmitic acid (C16:0), oleic acid (C18:1), alpha-linolenic acid (C18:3) are shown with respect to chain length and degree of unsaturation. The chemical formula is $C_{55}H_{98}O_6$.

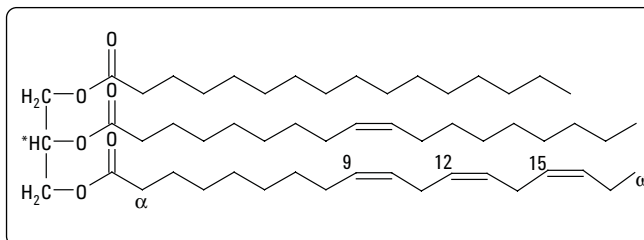


Figure 1. Typical triglyceride structure.

Experimental

Sample Preparation

The primary solution was prepared at a concentration of 10 mg/mL, in 2-propanol or 2:1 volume to volume MeOH/MTBE, and subsequently diluted to lower concentrations as needed. Injection volumes of 0.2-2 μ L were made into the LC/DAD system.

LC Method Details

LC Conditions

Agilent 1290 Infinity LC System binary pump G4220A,
Agilent 1290 Infinity LC System autosampler G4226A
Agilent Thermostatted Column Compartment G1316C with switching valve
Agilent 1290 Infinity LC System diode array UV/VIS detector G4212A with 10 mm path fiber optic flow cell

Columns: (See individual figures for specific usage)
Agilent ZORBAX SB-C18 RRHT, 3 mm \times 150 mm, 1.8 μ m
600 bar, p/n 829975-302
Agilent ZORBAX SB-C18 RRHD, 2.1 mm \times 100 mm, 1.8 μ m
1200 bar, p/n 858700-902
Agilent ZORBAX SB-C18 RRHD, 2.1 mm \times 150 mm, 1.8 μ m
1200 bar, p/n 859700-902
In some cases, columns were coupled to extend the length and resolution.

Column temp: 20 $^{\circ}$ C or 30 $^{\circ}$ C

Mobile phase: A = acetonitrile
B = isopropanol (IPA) or tert butyl methyl ether (MTBE) (See individual figures)

Flow rate: See individual figures

Gradient: The gradient conditions were either 20% to 60% IPA or 10% to 40% MTBE, based on the strong eluting strength of MTBE when compared to IPA. The gradient slope was maintained at 2.6% organic phase increase per column volume for IPA gradients and 2.0% with MTBE, altering gradient time and flow rate accordingly. This was determined by calculations using a modification of the Agilent Method Translator. [3]

UV Conditions

Monitoring 210, 220 and 230 nm, bandwidth 4 nm, reference wavelength off

Results and Discussion

A typical gradient separation of triglycerides using acetonitrile IPA gradient is shown in Figure 2.

Some general comments are appropriate about the conditions and chromatographic profile shown in Figure 2. While it would be ideal to consider less expensive methanol as the weak eluent, introduction of methanol or denatured ethanol

containing methanol has consistently shown a dramatic reduction in the overall resolution of the triglycerides. The significant increase in operating pressure, when running the gradient from acetonitrile to IPA, is clearly limiting and undesirable. Increasing the operating temperature of the column as a means of reducing solvent viscosity has proven to be undesirable because the chromatographic resolution tends to collapse as temperature increases.

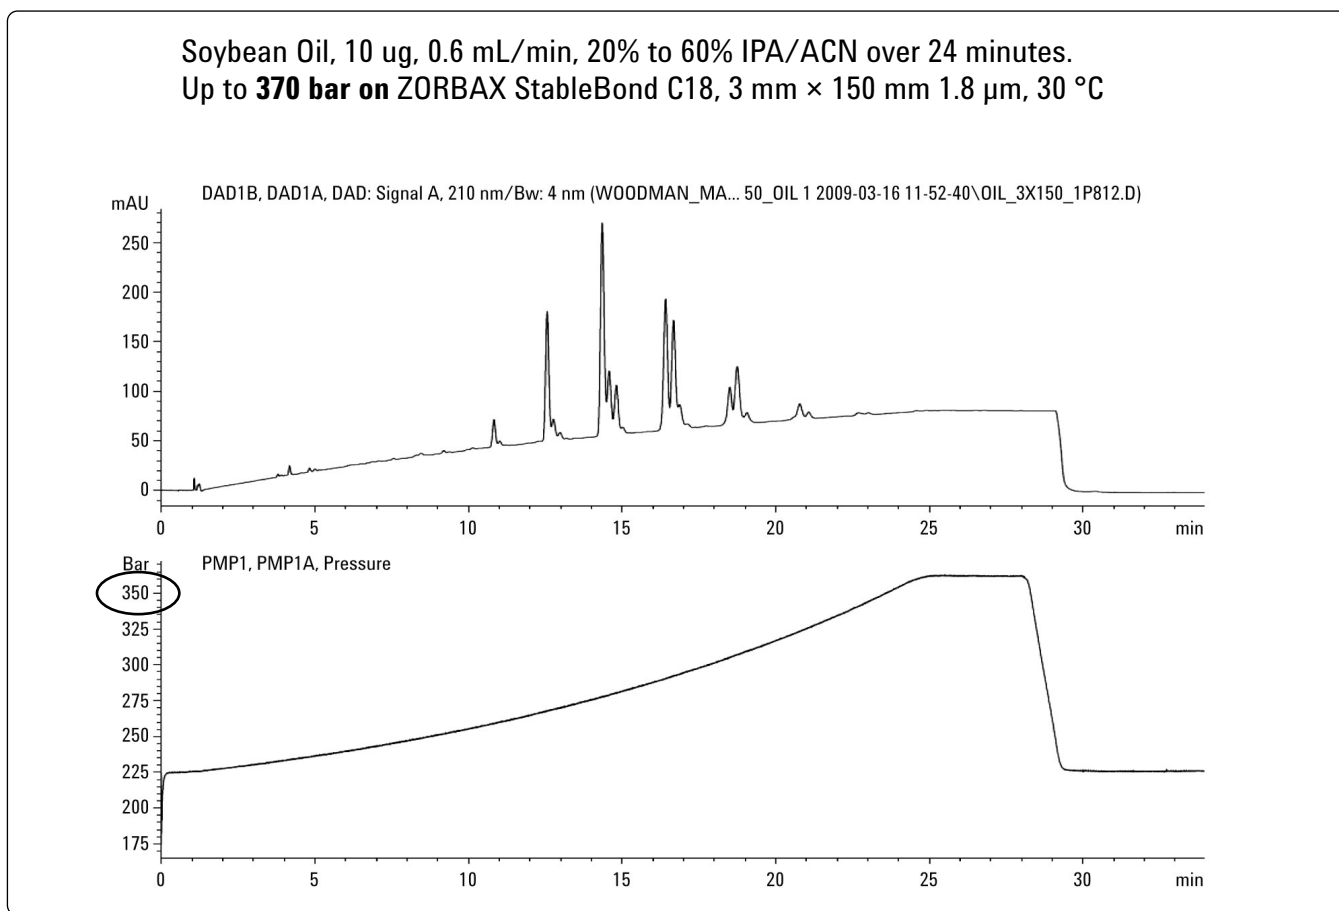


Figure 2. A 210-nm UV chromatogram of soybean oil sample on a 3 mm × 150 mm ZORBAX Rapid Resolution High Throughput (RRHT), 1.8 μm column, upper panel. System pressure trace showing the general progress of the gradient elution, lower panel. Flow rate 0.6 mL/min, gradient time 24 min. Strong solvent, isopropanol. The chromatogram demonstrates the typical difficulty encountered with this type of separation, which is small clusters of chromatographically similar triglycerides. These clusters are not positional isomers of the same carbon number and degree of unsaturation, rather a mixture of various chain lengths and number of double bonds as shown by mass spectrometric evaluation.

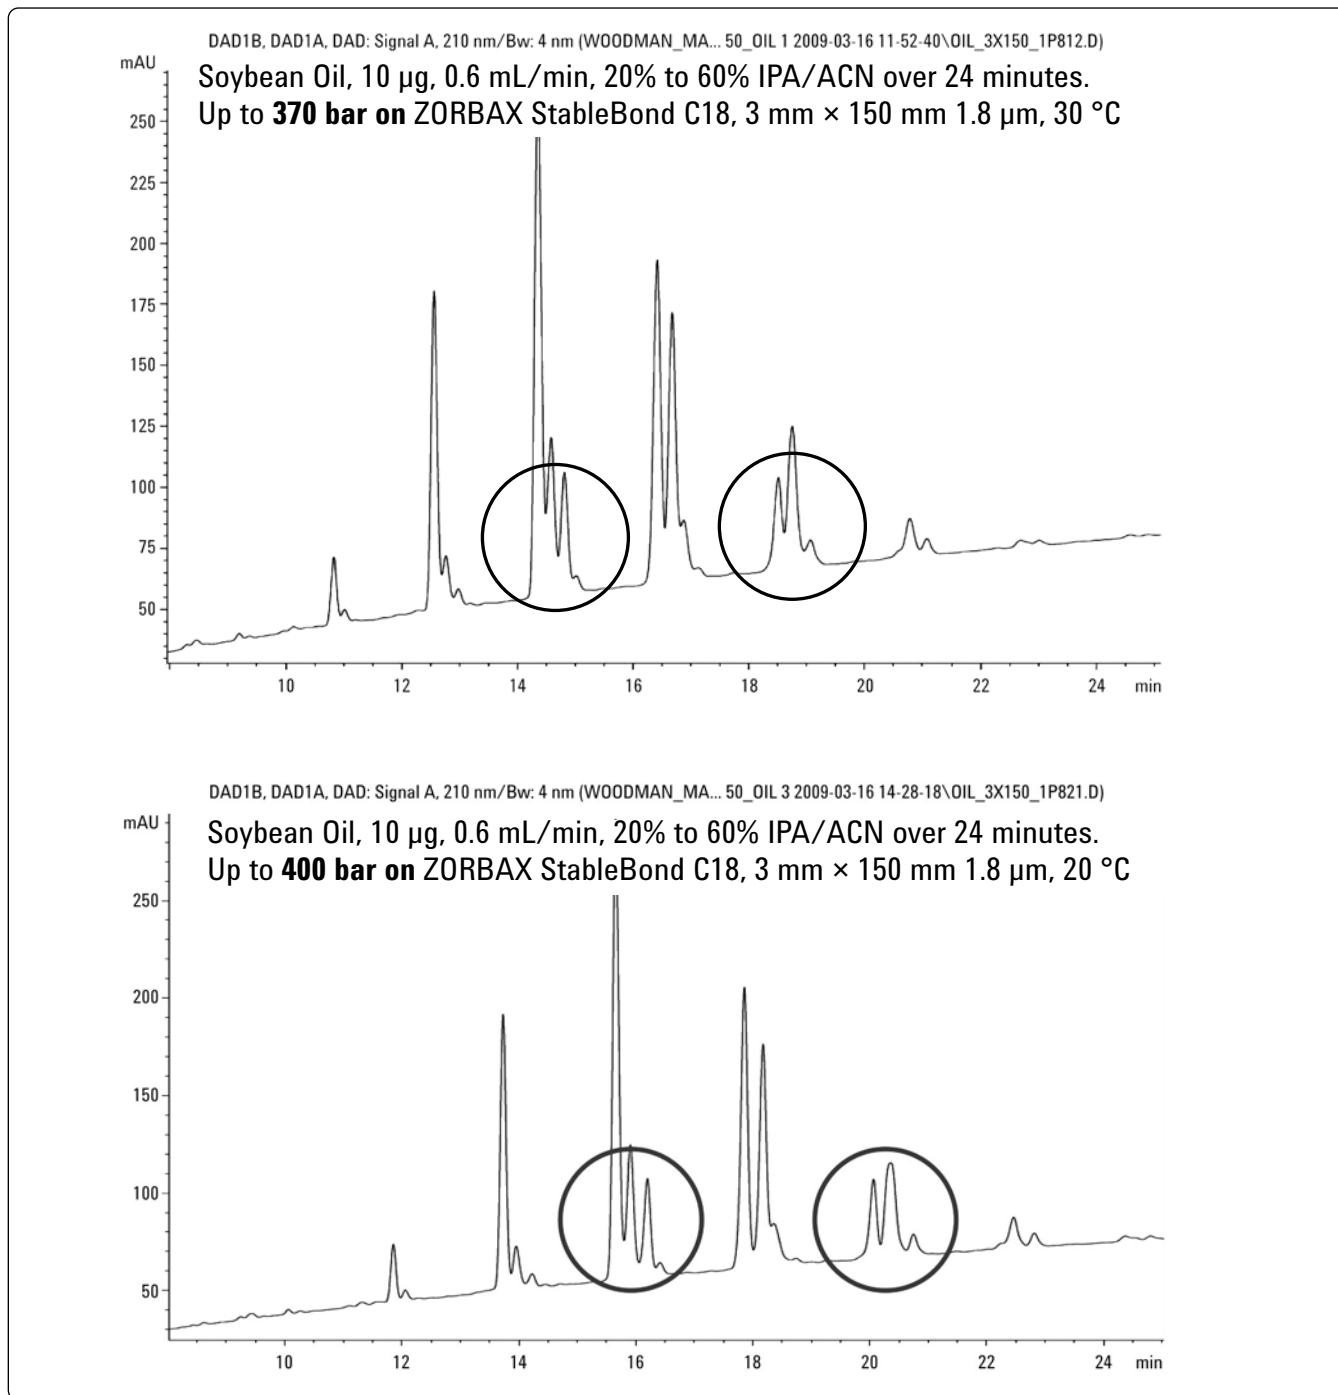


Figure 3. An expanded presentation of the chromatogram shown in Figure 2 at 30 °C, upper panel, compared with the same conditions in Figure 2 operating the column at 20 °C.

In Figure 3 we see the improvement achieved by operating the separation at 20 °C rather than 30 °C. The operating pressure increase is approximately 10% at the lower temperature. While many of our separations have been performed at 30 °C

as a compromise between separation and operating pressure, the availability of the Agilent 1290 Infinity LC System with increased operating pressure capability has allowed us to reduce the temperature to 20 °C and demonstrate a usable improvement in separation.

Soybean Oil, 10 µg, 0.29 mL/min, 20% to 60% IPA/ACN over 27 minutes.
Up to **760 bar** on ZORBAX StableBond C18, 2.1 mm × 250 mm 1.8 µm, 20 °C

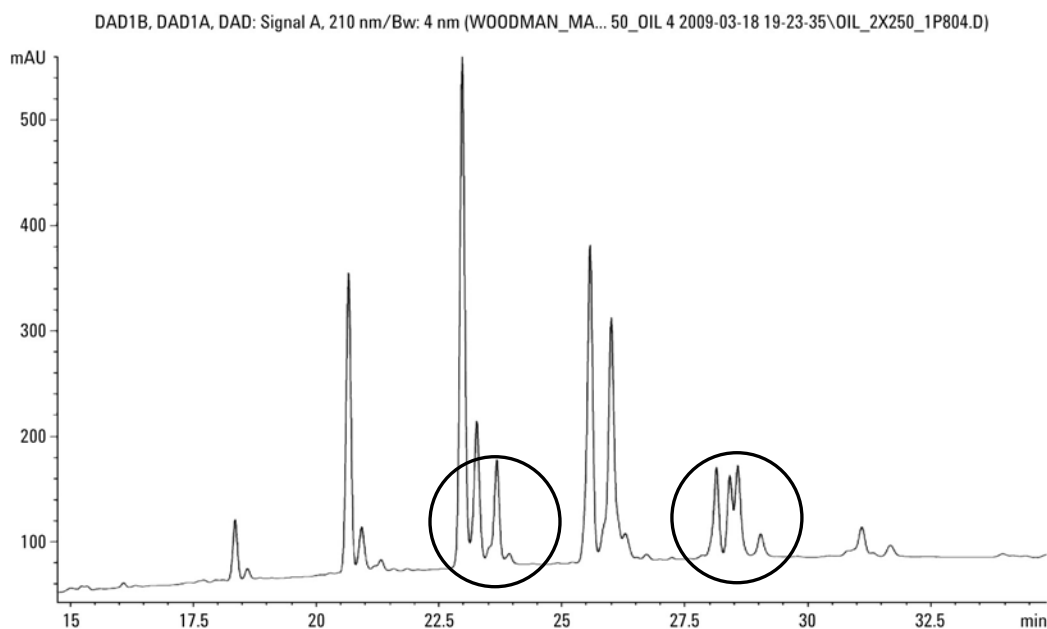


Figure 4. Analysis of the soybean oil sample on an Agilent ZORBAX StableBond C18 column, 2.1 mm × 250 mm, 1.8 µm, (150 mm in series with 100 mm) prepared for operation at 1200 bar pressure limit. Flow rate 0.29 mL/min, gradient time 27 min. Maximum observed pressure 760 bar.

In Figure 4, we see that increasing the length of the column has resulted in a significant increase in the resolution of some of the observed components. To further increase resolution, it would be practical to explore longer columns or explore alternative mobile phase or column chemistries. As with most very high performance separations, rate-limiting features tend to include operating pressure, operating temperature, and maximum flow rate. The triglyceride separations evaluated thus far have not been receptive to operation at higher column temperatures or higher flow rates, presumably because of their

relatively high molecular weight and flexible organic structure. Even when gradient slope translations are carefully made to ensure organic strength consistency from method to method, operating at higher flow rates has consistently shown degradation of the overall separation. Because the isopropanol has significantly high viscosity and high pressure, it seemed appropriate to consider other non-polar solvents that are miscible with acetonitrile and friendly to low UV detection, as a substitute for isopropanol.

Soybean Oil, 10 µg, 0.29 mL/min, 10% to 40% IPA/ACN over 27 minutes.
Up to **440 bar** on ZORBAX StableBond C18, 2.1 mm × 250 mm 1.8 µm, 20 °C

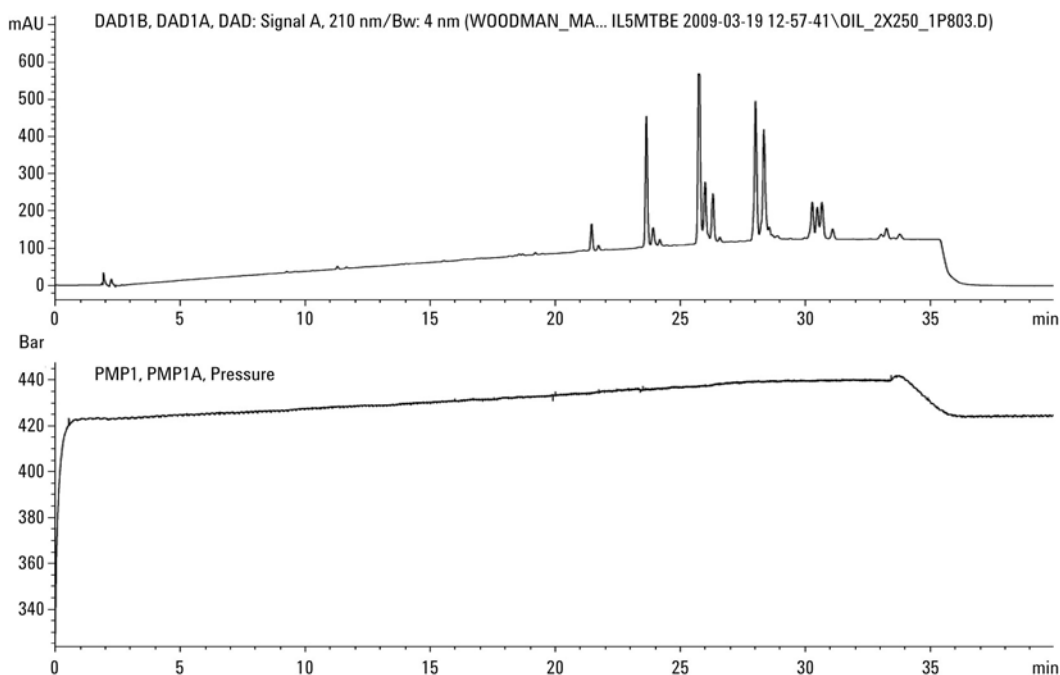


Figure 5. By substituting MTBE for isopropanol with otherwise the same conditions as Figure 4, and then re-optimizing the gradient for the significant increase in eluting strength of MTBE, we arrive at a new set of operating conditions where there is only a small difference in operating pressure over the gradient run. Flow rate 0.29 mL/min, gradient 27 min for 10% to 40% MTBE, maximum observed pressure 440 bar.

In Figure 5, the change to MTBE and subsequent readjustment of the gradient resulted in a separation that was very comparable to the original isopropanol separation, however at a much lower maximum operating pressure. In view of the prior evidence and comments regarding increased temperature or flow rate resulting in degraded separation, it seemed that the most appropriate way to take advantage of the new operating pressure capability of the Agilent 1290 Infinity LC

System was to continue to increase the column length. The Agilent 1290 Infinity LC System and associated ZORBAX chemistries are capable of operating pressures up to 1200 bar, or approximately 18,000 psi. To ensure robust and rugged system operation many users typically specify the upper pressure limit for a method at a value less than 80% of the rated operating pressure.

Soybean Oil, 30 µg, 0.29 mL/min, 10% to 40% MTBE/ACN over 43 minutes.
Up to **730 bar** on ZORBAX StableBond C18, 2.1 mm × 400 mm, 1.8 µm, 20 °C

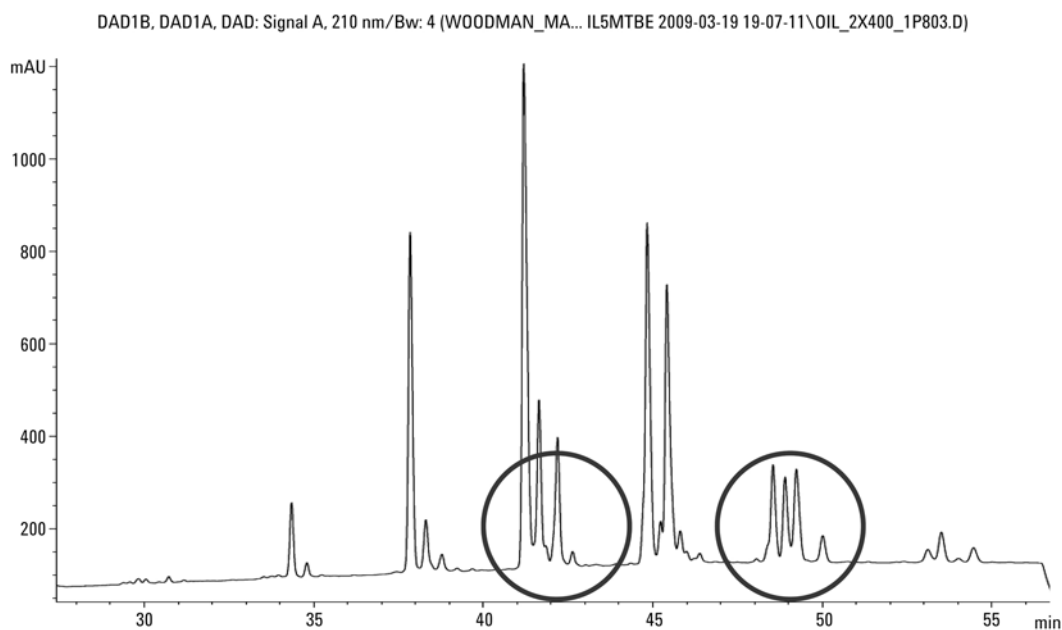


Figure 6. Separation of the soybean oil sample on a 2.1 mm × 400 mm ZORBAX StableBond C18, 1.8 µm 1200 bar columns (150 mm + 150 mm + 100 mm in series). Flow rate 0.29 mL/min gradient time 43 min, for a gradient of 10% to 40% MTBE. Maximum operating pressure 730 bar at 20 °C.

As shown in Figure 6, having previously optimized the column temperature, operating flow rate and gradient slope for the best possible balance between resolution and analysis time, and after investigating a variety of solvents as candidates for both the weak solvent and strong solvent choice, we are left with an ultimate opportunity to operate on a very long column set of 1.8 µm particle size columns under conditions ideal for the separation of this group of triglycerides. With an operating pressure of only 730 bar, which is about 60% of the rated capability of the Agilent 1290 Infinity LC System, it is clearly possible to consider even longer column lengths or a further reduction in the operating temperature as both of these seem promising in terms of delivering even higher resolution out of the mixture.

The separation with MTBE or isopropanol can be adapted for use with a mass spectrometer as one of the detectors. In previous studies (see www.Agilent.com/chem ASMS 2009 for a poster on this subject) we have been able to demonstrate the capability of quickly and confidently identifying the composition of many of the triglycerides found in this and other samples. For optimum electrospray performance in the non-aqueous, non-buffered environment it was useful to do post UV detector addition of a mixture of methanol and water with ammonium formate buffer to enhance ionization and to ensure a consistent ability to preserve the molecular ion into the mass spectrometer. It has been shown by McIntyre [4] that the presence of ammonium formate in the mobile phase significantly improves the probability that a molecular ion will be formed and preserved in the mass analyzer portion of a mass spectrometer.

Conclusions

Using the Agilent 1290 Infinity LC System, we were able to easily demonstrate UHPLC capabilities well within the operating range of the instrument. The significantly enhanced resolution afforded by long sub-2 micron particle size columns in the sub-ambient column compartment environment will contribute significantly to our understanding of the major and minor composition of this sample and other similar materials. This should significantly enhance the contribution of liquid chromatography to the understanding of seed oil composition, the role of triglycerides in metabolism, and the area of lipidomics where great interest has been directed on the LC separation coupled to time-of-flight high-resolution mass spectrometry (LC/TOF).

References

1. E. G. Perkins, "Analyses of Fats, Oils, and Derivatives," AOCS Press, 1993
2. http://en.wikipedia.org/wiki/File:Fat_triglyceride_short-hand_formula.PNG
3. (<http://www.chem.agilent.com/en-US/products/instruments/lc/pages/gp60931.aspx>)
4. D. McIntyre, "The Analysis of Triglycerides in Edible Oils by APCI LC/MS", May, 2000 Agilent Technologies publication 5968-0878E

For More Information

For more information on our products and services, visit our Web site at www.agilent.com/chem.

www.agilent.com/chem

Agilent shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Information, descriptions, and specifications in this publication are subject to change without notice.

© Agilent Technologies, Inc., 2009
Printed in the USA
August 3, 2009
5990-4292EN



Agilent Technologies